


An LC-MS/MS Method for Simultaneous Measurement of Five Antimicrobial Drugs (Vancomycin, Gentamicin, Amikacin, Linezolid and Teicoplanin) for TDM.

Martini A. (1), Mirri P. (1), Casetta B. (2), Albertini M. (2), Sandroni F. (2), Clerici P. (1)
(1) ASST Ovest Milanese – Legnano, Italy; (2) B.S.N. – Castelleone, Italy.

Introduction

LC-MS/MS is pivotal for measuring any xenobiotic molecule in biological fluid. Besides its incontrovertible advantages there is usually the need to rely on an isotopically-labeled internal standard for mitigating any matrix and/or recovery issues. Nonetheless these labeled compounds can pose availability and cost constraints when related to newly-introduced pharmaceutical drugs. Hereby we present the results achieved by a new protocol for measuring the nowadays most used antibiotic drugs.

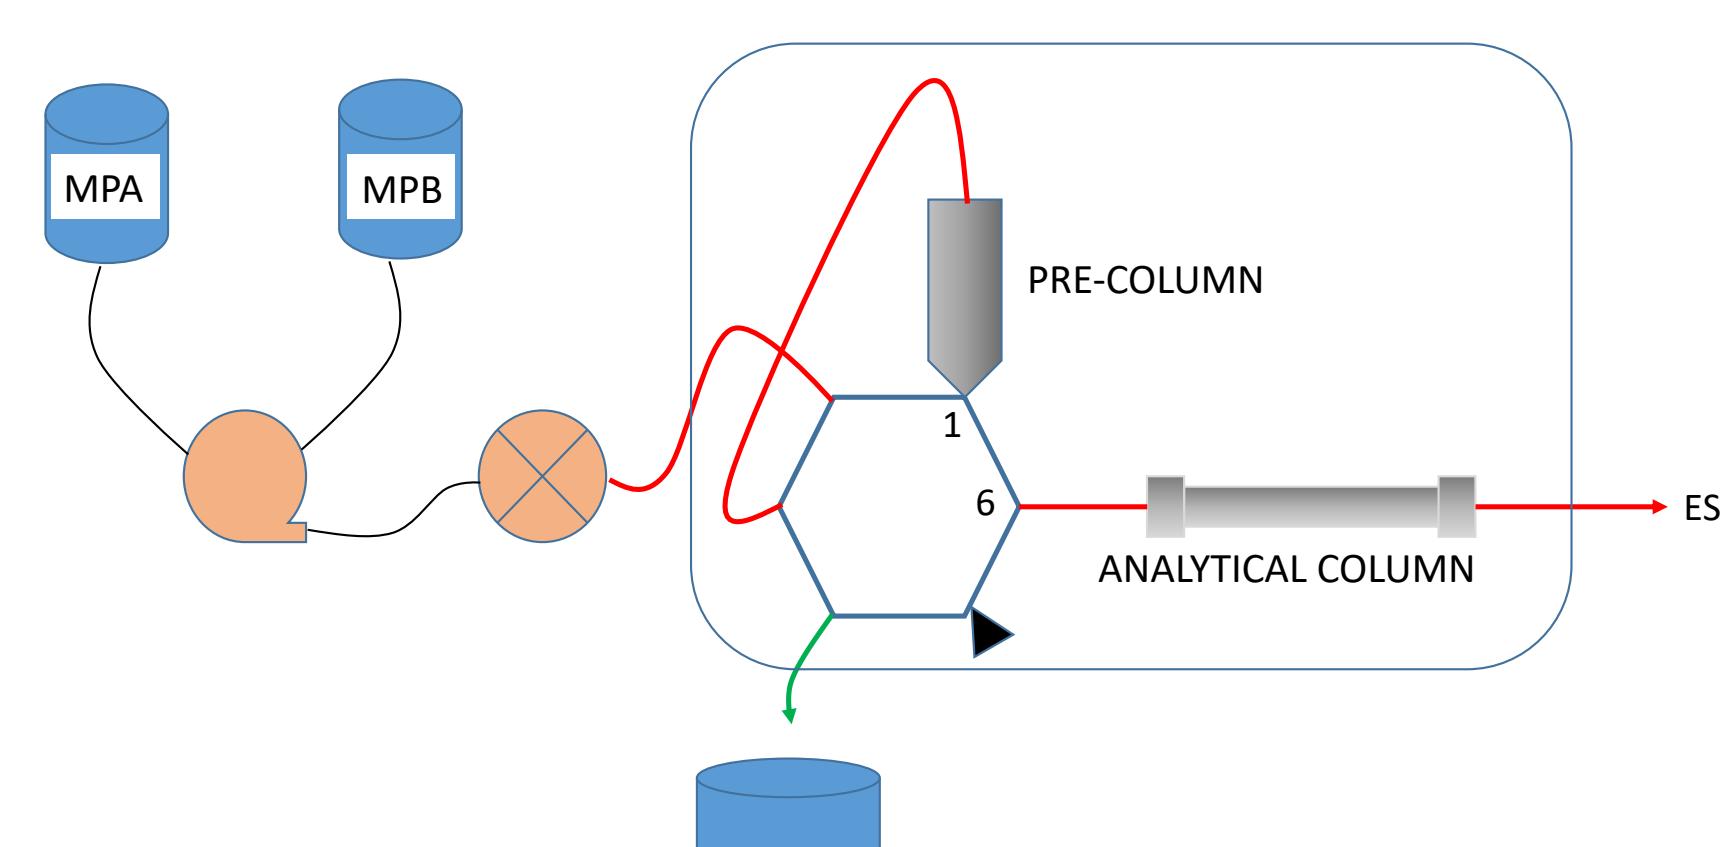

Method

Method relies on a commercially available kit centered on:




- A protein precipitation sample preparation.
- A special plumbing for a quick on-line sample clean-up.
- The addition of a single internal standard, not an isotopologue.

Results

- Verified through post-column analyte addition as ion-suppression impact is negligible.
- Adequate linearity and LLOQ for all the drugs and good precision.

	AMIKACIN	VANCOMYCIN	TEICOPLANIN	GENTAMICIN	LINEZOLID
LLOD (ng/ml)	6,9	25,1	13,7	0,94	2,1
LLOQ (ng/ml)	23,0	83,7	45,7	3,13	7,2
Linearity (μ g/ml)	1 - 50	2 - 100	2 - 100	0,2 - 10	1 - 50

ANALYTE	LEVEL	Avg Conc. (μ g/ml)	CV% Intra	CV% Inter	CV% Total
Amikacin	Low	2,5	5,6%	8,1%	9,8%
	Medium	6,3	7,1%	7,4%	10,3%
	High	32,7	6,0%	7,9%	9,9%
Vancomycin	Low	4,4	5,2%	10,0%	11,3%
	Medium	11,7	5,5%	11,0%	12,3%
	High	56,7	4,3%	8,8%	9,8%
Teicoplanin	Low	3,7	4,4%	10,4%	11,3%
	Medium	10,4	4,5%	8,4%	9,5%
	High	49,9	3,8%	6,7%	7,7%
Gentamicin	Low	0,47	4,5%	6,1%	7,6%
	Medium	1,22	5,9%	8,1%	10%
	High	6,19	3,8%	8,9%	9,7%
Linezolid	Low	3,0	6,5%	9,0%	11,1%
	Medium	7,8	2,1%	6,8%	7,1%
	High	30,8	1,9%	7,2%	7,4%

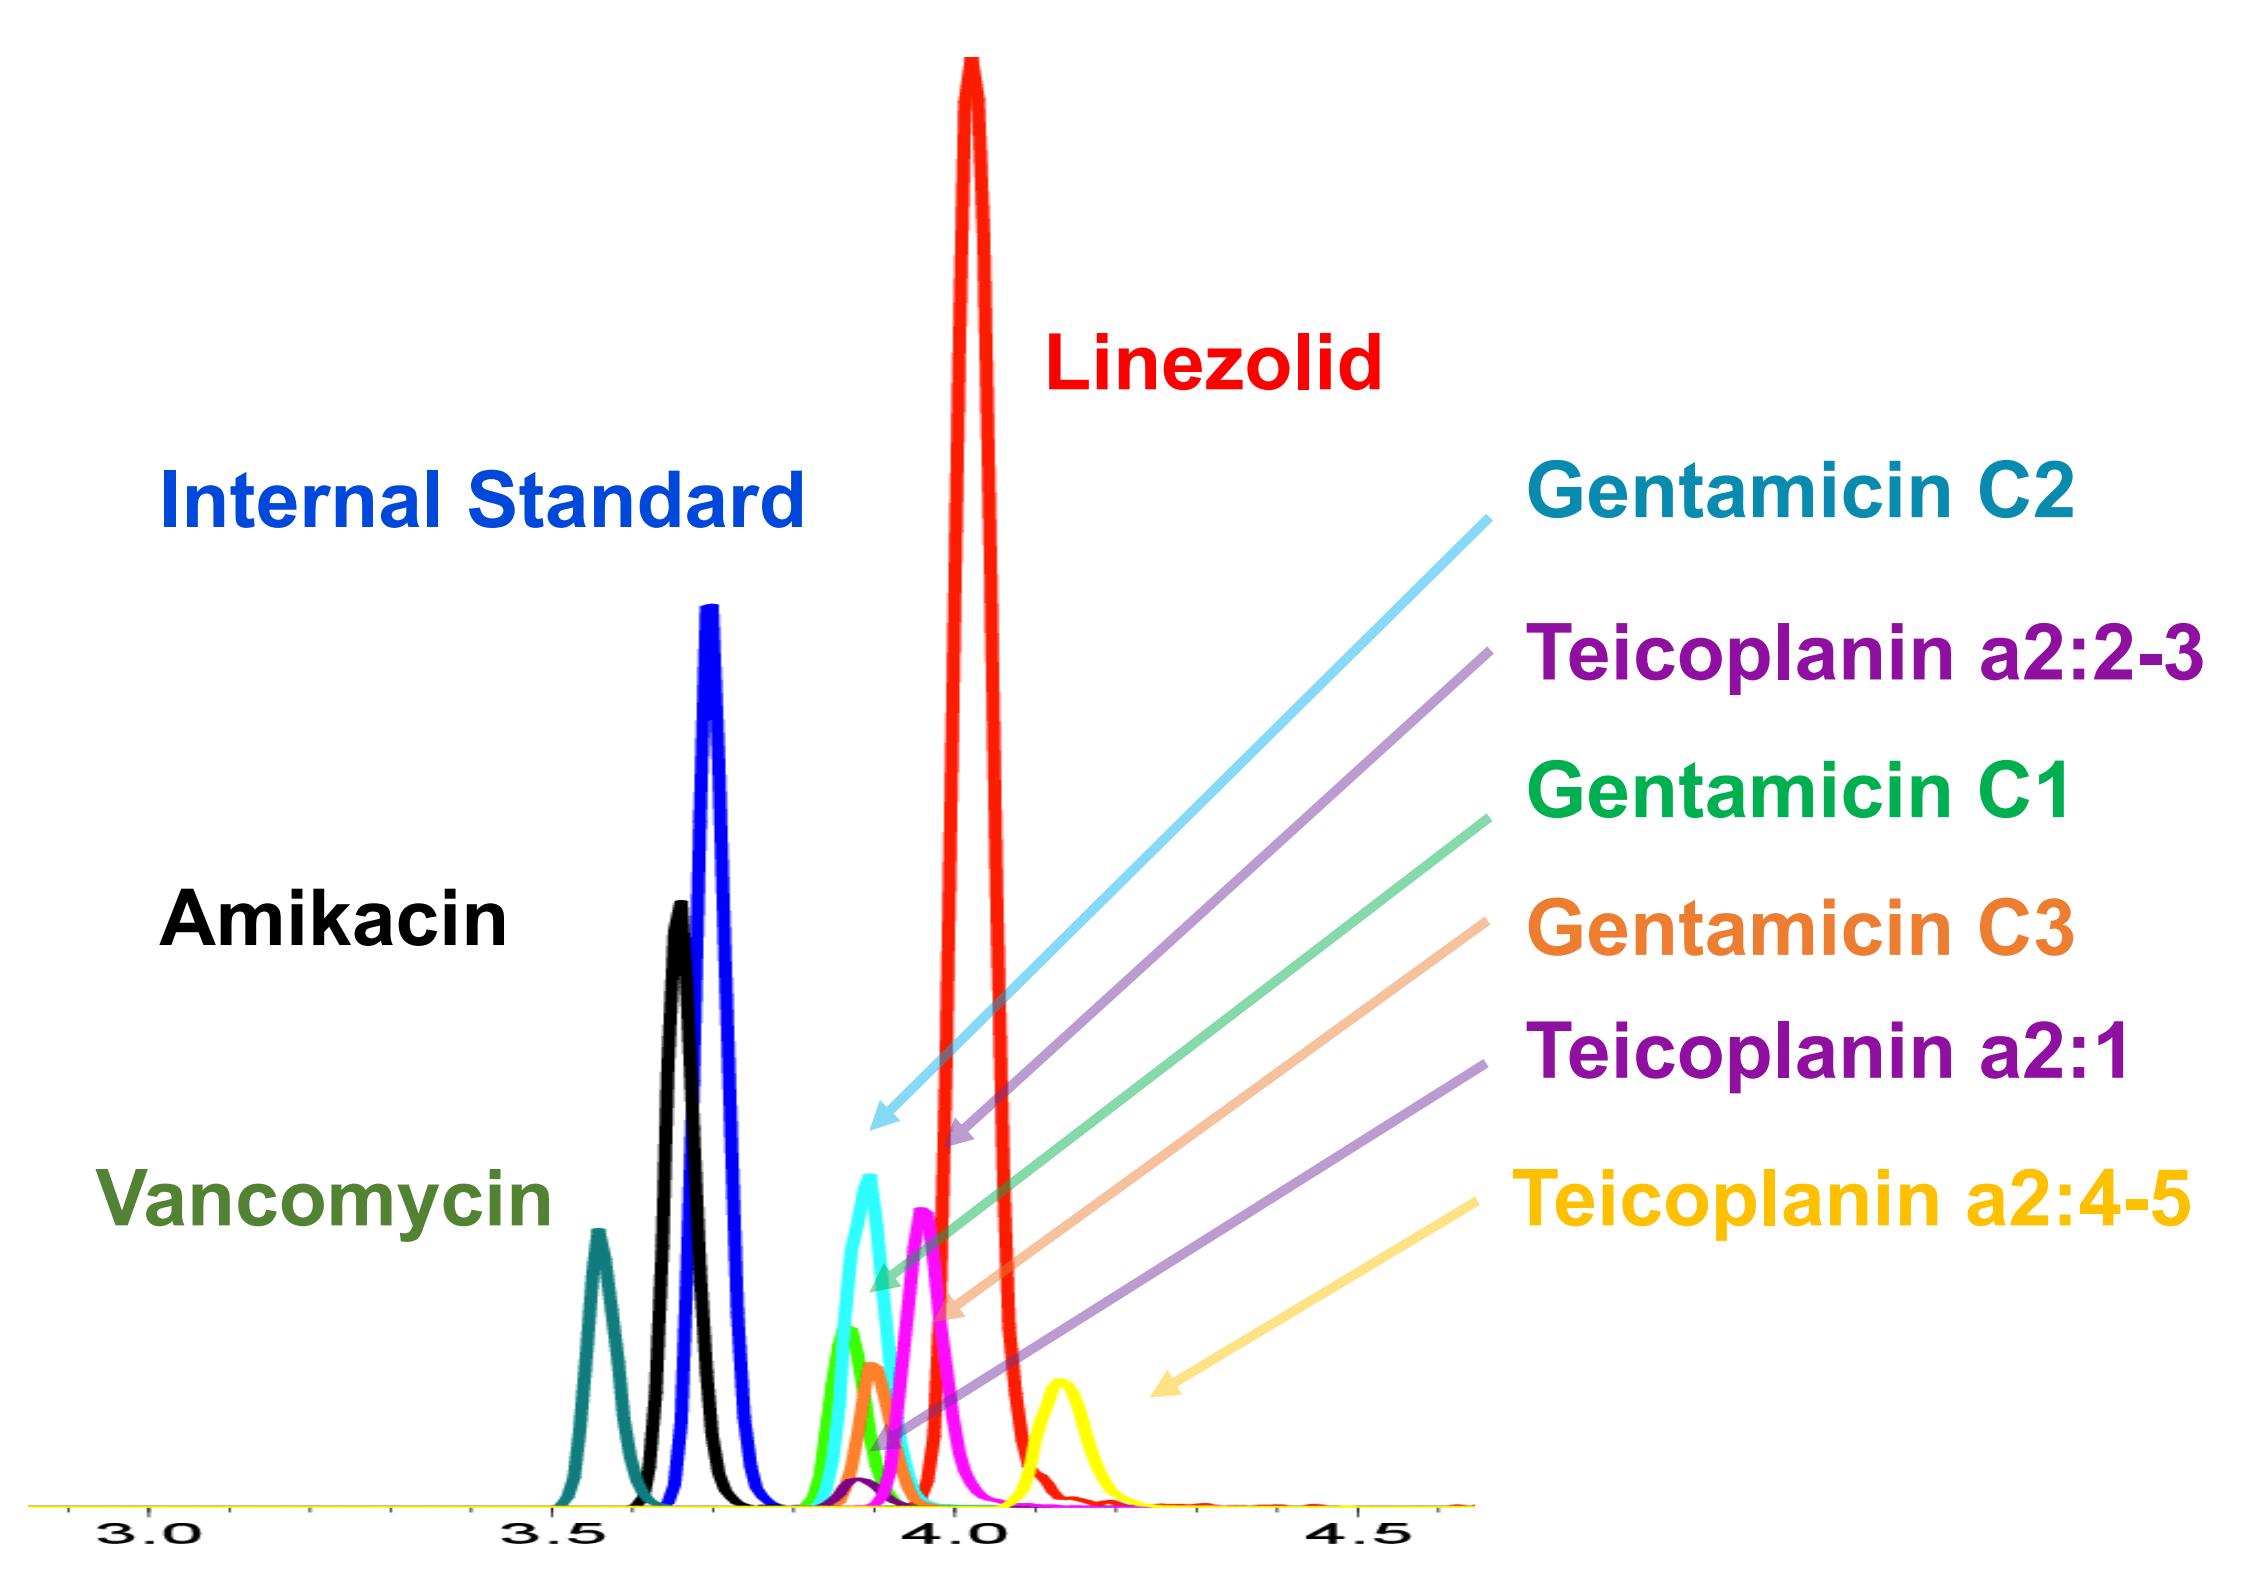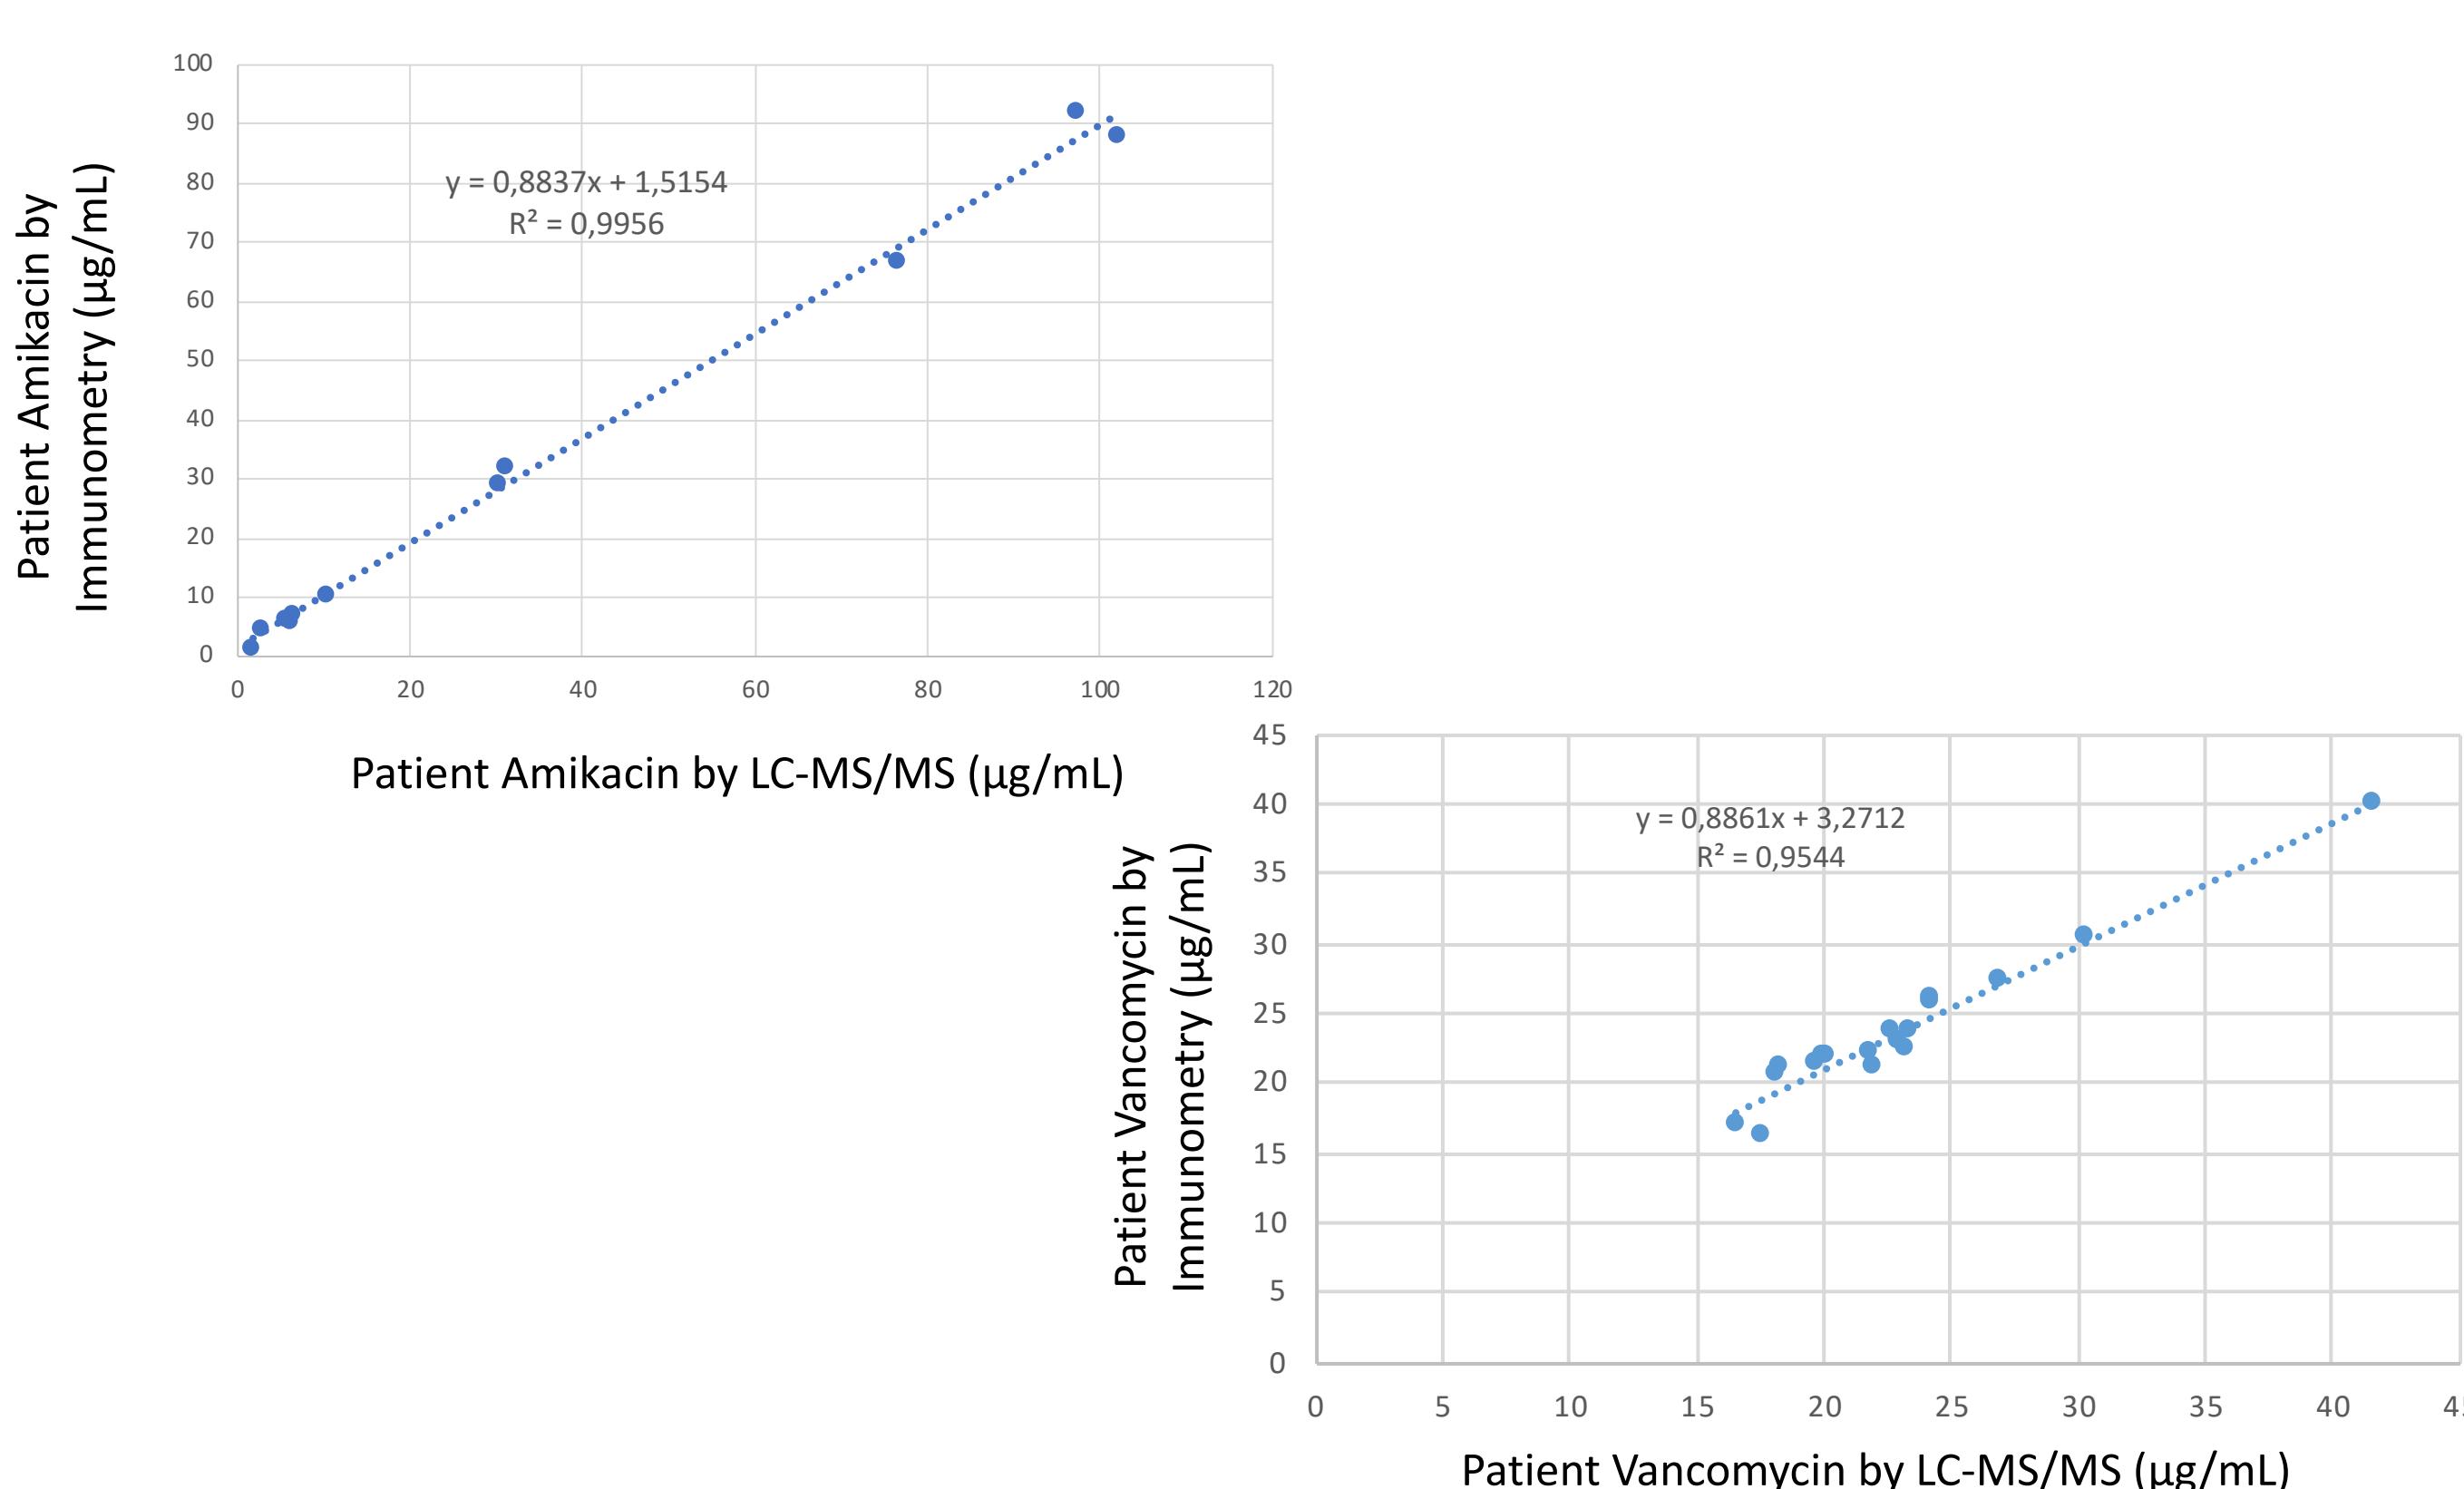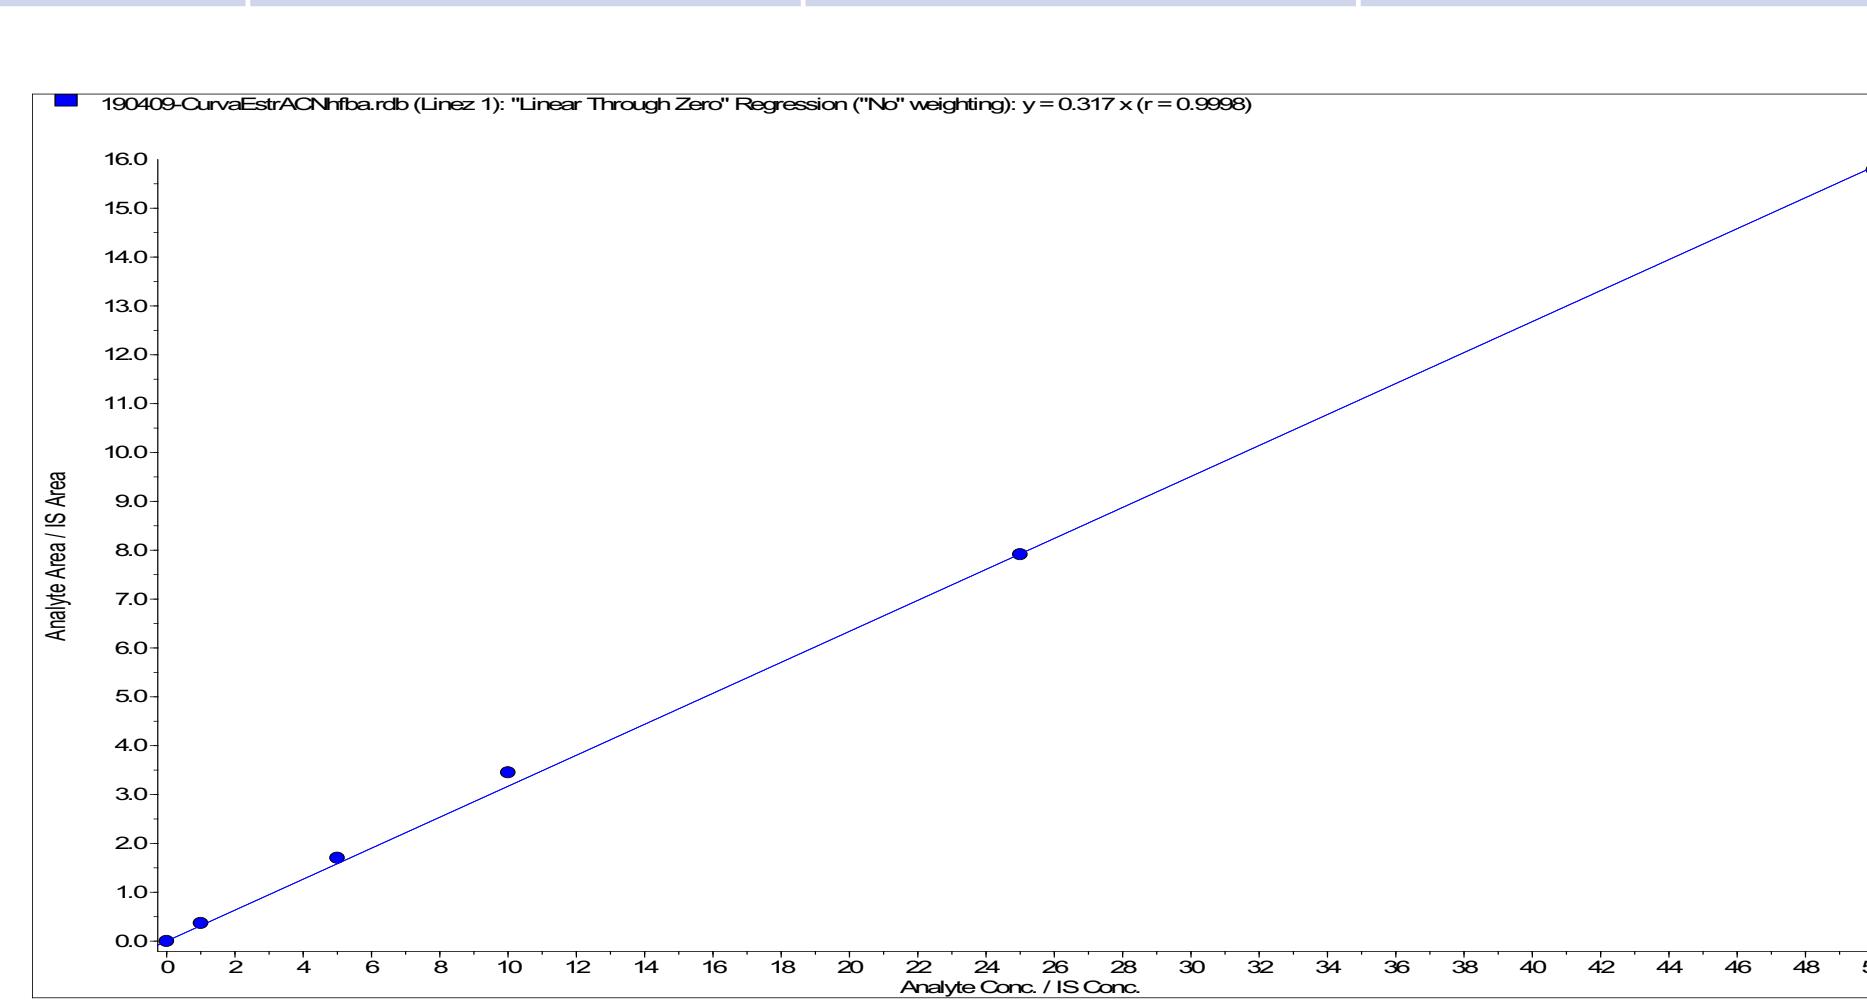

Conclusion

- Good correlation with immunometry on patient samples (slope = 0.89 for measured Amikacin and Vancomycin).
- Homologues of Gentamicin and Teicoplanin resolved.

